

# Volumetric Sample Cutter



## Site Preparation Guide

# Table of Contents


Table of Contents .....	1
Ideal Setup .....	2
System Components.....	3
Instrument Measurements .....	4
Utility Requirements.....	5
Site Preparation Checklist .....	6
TA Instrument Offices.....	7

# Ideal Setup



## IDEAL PLACEMENT AND BENCH MEASUREMENTS

Select a location with adequate floor space and a rigid laboratory bench that is level and is in a vibration-free environment.

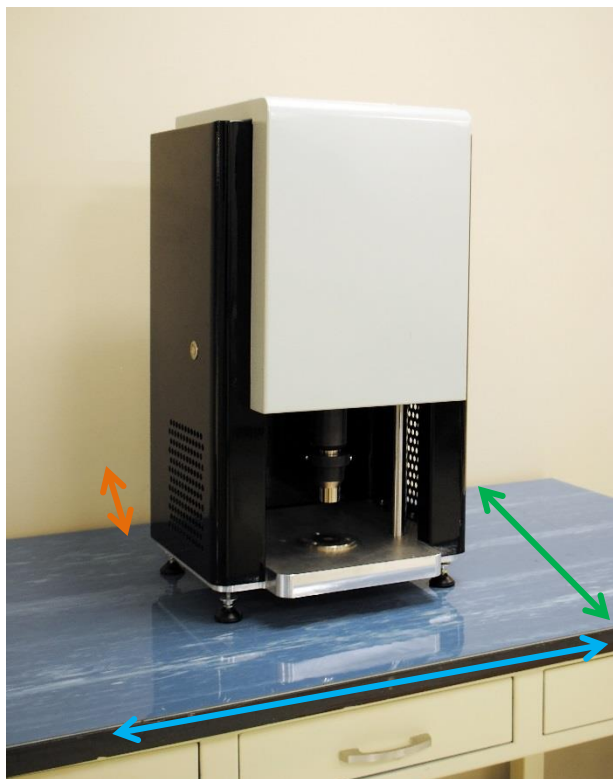

Bench length: 70 cm (27.5 in)


Bench depth: 80 cm (31 in) min.

Distance from the wall: 20 cm (8 in) min.

# System Components



## MAIN SYSTEM COMPONENTS

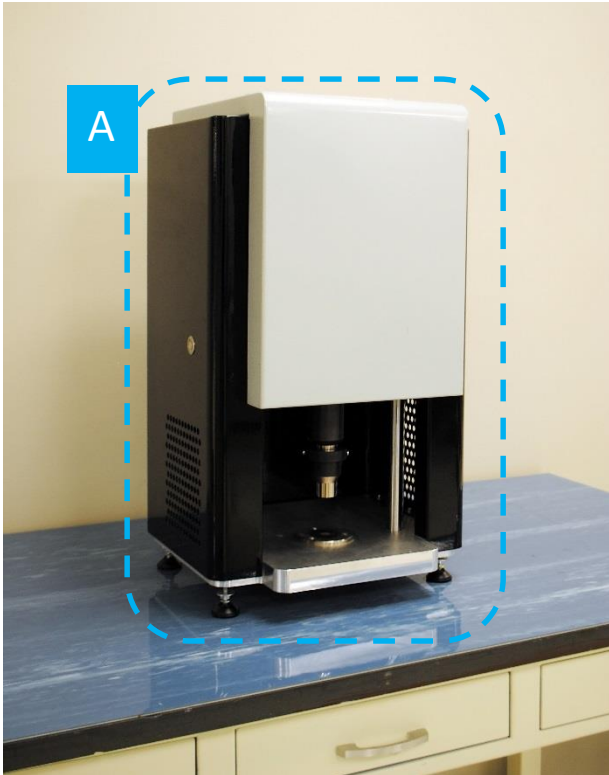

**A. Instrument**

# Instrument Measurements



## MAIN INSTRUMENT



Height: 68 cm (27 in)

Width: 40 cm (16 in)

Depth: 43.5 cm (17 in)

Weight: 55 kg (121 lbs)

# Utility Requirements



## POWER

- 1 electrical socket 230/110 VAC 50/60 Hz available for instrument that provides minimum 3.15 A and is protected against voltage fluctuations and electrical noise
- Separate and secure additional power supply for PC and monitor



## GAS

- 6.0 bars (87 psig) (optional booster up to 8.0 bars)



# TA Instruments Offices

For information on our latest products, contact information, and more, see our website at:  
<http://www.tainstruments.com>.

To find your local TA Instruments office and contact information, visit  
<http://www.tainstruments.com/contact/ta-directory/>

TA Instruments – Waters LLC  
Corporate Headquarters  
159 Lukens Drive  
New Castle, DE 19720  
USA

Telephone: 302-427-4000

Fax: 302-427-4001

Email: [info@tainstruments.com](mailto:info@tainstruments.com)